Pura™ GETTING STARTED GUIDE (For self-testing)

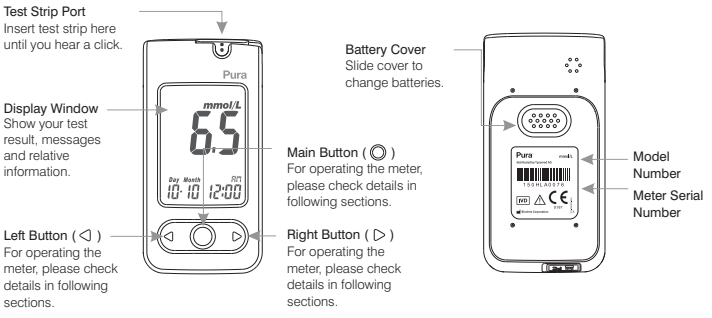
Test Strip Port
Insert test strip here until you hear a click.
Display Window
Show your test result, messages and relative information.
Left Button (◁)
For operating the meter, please check details in following sections.
Main Button (◎)
For operating the meter, please check details in following sections.
Right Button (▷)
For operating the meter, please check details in following sections.
Battery Cover
Slide cover to change batteries.
Model Number
Meter Serial Number

Front View of Meter **Back View of Meter**

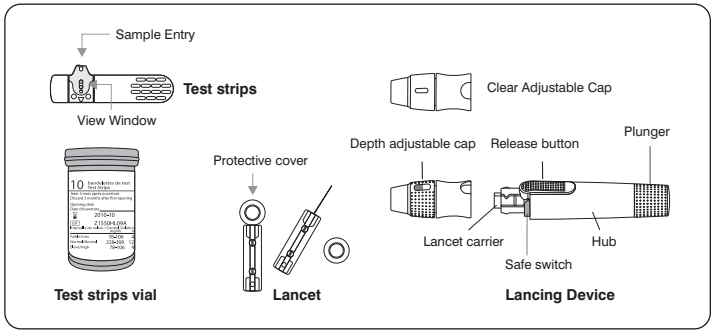

1 Batteries Installation

1) Turn the meter over. Press and push batteries cover to open.
2) Install the battery. Be sure to put battery in correct direction.
3) Slide the battery cover back until it snaps into place.

2 Setting Up Your Meter - Setting the Date, Time and Unit

1) Press and release main button " ◎ " to turn on the Meter.
2) Press and hold main button " ◎ " for 7 seconds until you go into the setting mode. Before you go into setting mode, the meter will turn off first. Please keep pressing it until you go into the setting mode. The year will flash.
3) Press left button " ◁ " or right button " ▷ " to change the year.
4) Press main button " ◎ " to confirm the year and move to month setting.
5) Repeat steps 3 and 4 to change the date, time format, hour, minute, volume and measurement unit. After pressing the main button to confirm the measurement unit, your set-up has been finished.



> NOTE
> - Suggest not to use this meter close to source of strong electromagnetic radiation, to avoid interference with proper operation.
> - Suggest to keep meter free of dust, water or any liquid.

3 Preparing the Lancing Device

1) Hold the adjustable cap in one hand and hold the hub in the other hand. Bend the cap towards the down side. When a gap appears between the cap and hub, pull them off in opposite directions.
2) Pull off the depth adjustable cap.
3) Insert a new disposable lancet firmly into lancet carrier.

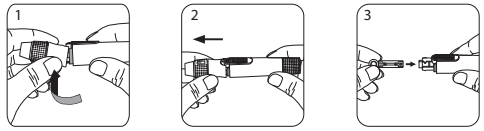

4) Twist off and set aside the protective cover of the disposable lancet.
5) Replace the depth adjustable cap.
6) Choose a depth of penetration by rotating the top portion of the depth adjustable cap until the setting depth matches the window. Settings are based on skin type
   " ▭ " for soft or thin skin;
   " ▭ " for average skin;
   " ▭ " for thick or calloused skin.
7) Hold the hub in one hand and pull on the plunger in the other hand. The device will be cocked. Release the plunger, it will automatically move back to its original position near the hub.

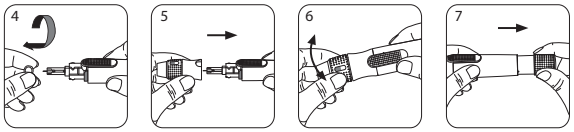

4 Performing a Test

1) Wash and dry your hands. Take one strip from the vial. Close the vial cap immediately.
2) Insert the strip into the strip port on meter with the indication symbol facing up. Push the strip in until it snaps and stops. The meter will automatically detect code number.
3) When you see the flashing blood drop, hold the lancing device to side of your fingertip and press the release button.
4) Gently squeeze your fingertip to get a drop of blood. Our Meter only needs a tiny blood sample. We suggest to get a blood sample size around 0.7~2.0μL to test it. Please don't squeeze too much blood. Too much blood (>4.0μL) might contaminate the meter. Not enough blood (<0.7μL) might cause inaccurate result.

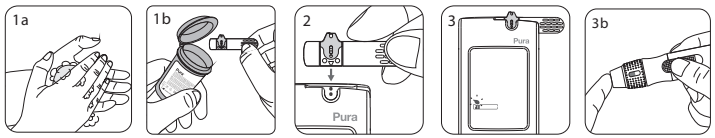

Sample Size Example



5) Touch and hold the drop to the edge of sample entry until you hear a " beep " and the view window is totally filled with blood. If the view window is not totally filled with blood or the test does not start. Then discard the test strip and repeat the test with a new test strip.
6) You will see the countdown mode on the screen. After 11 seconds, the test result appears. For more information about your test results, please see your User Manual.

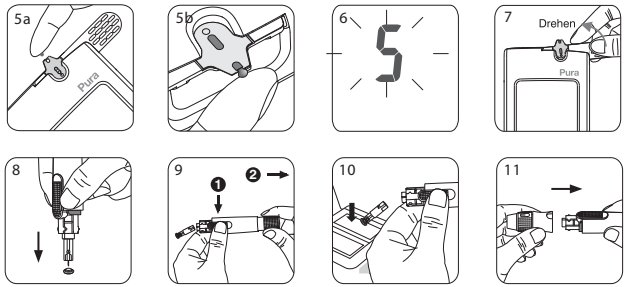

7) Remove the test strip from meter. Please follow the local regulation and discard the used strip properly.
8) Pull off the depth adjustable cap. Without touching the used disposable lancet, stick the lancet tip into the protective cover.
9) Hold the release button in one hand and pull on the plunger in the other hand will safely eject the used disposable lancet.
10) Discard the used disposable lancet into an appropriate puncture-proof or biohazard container.
11) Replace the depth adjustable cap after finishing the test.

Alternative site testing-palm or forearm blood sampling

1. Choose clear cap (AST cup) and follow step1 to step 5.
2. Massage the puncture area of palm or forearm for a few seconds.
3. Immediately after massaging the puncture area, press and hold the lancing device with the clear cap against palm or forearm.
4. Then press the release button.
5. Continue holding the lancing device against palm or forearm and gradually increase pressure for a few seconds until the blood sample size is sufficient.
6. Follow step 9 to discard the used disposable lancet.

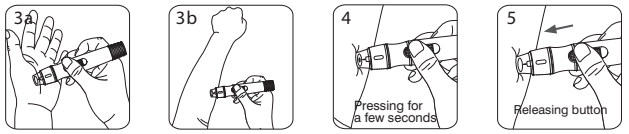

For more information on how to use your meter and understand your test results, please see the User Manual.

Distribution France
Ypsomed SAS
18-20 Rue Soleillet
75020 PARIS
Tél. 015870 2000
Fax 015870 2001
N°Vert : 0800 883058

Distribution UK
GBUK Healthcare
Blackwood Hall Business Park
North Duffield, Selby, N. Yorks, YO8 5DD
Service No. +44 (0)1757 288587
www.gbukhealthcare.com

BIONIME CORPORATION
694, Renhua Road, Dali City,
Taichung County,
Taiwan 412

EC REP
Bionime GmbH
Tramstrasse 16
CH-9442 Berneck
Suisse / Switzerland

CE 0197
101-3GM550-090
FR+EN